

Newborn Baby Check-Up™ DOLL

AGES 3 AND UP



Kenner®

© 1996 HASBRO, INC.
Pawtucket, Rhode Island 02862.
All Rights Reserved.

MADE IN CHINA

1

Remove screw from battery compartment door on bottom of case using a Phillips head screwdriver. Add two "AA" alkaline batteries (not included). Included is a replaceable "PR-4" bulb. Replace battery compartment door and screw it closed.

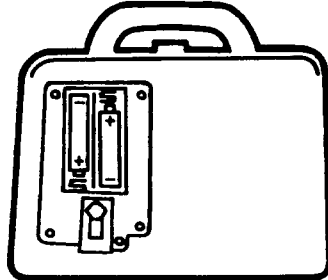

CAUTION: To avoid battery leakage, (1) Be sure to insert the batteries correctly and always follow the toy and battery manufacturer's instructions. (2) Do not mix old and new batteries or alkaline, standard (carbon-zinc) or rechargeable batteries. (3) Always remove exhausted or dead batteries from the product.


2

Pretend to scan your baby to get an x-ray.




3


Slide film into viewer. Turn on switch to take a look at her X-rays. One film shows your baby is OK and the other shows she needs you to take care of her.

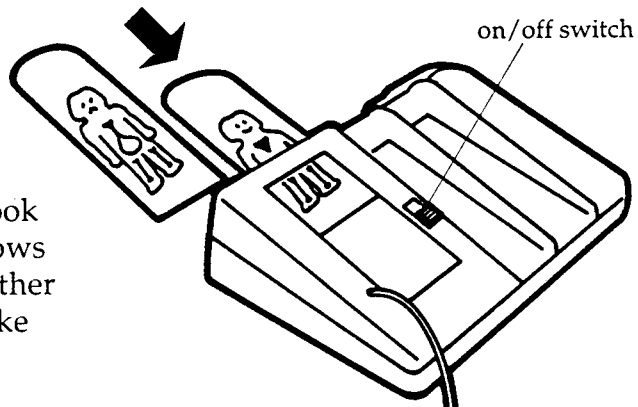

4

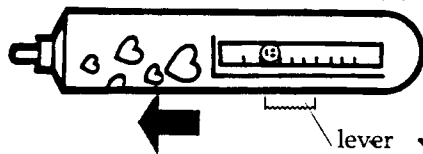

Check if your baby needs some medicine. Slide the lever on the thermometer towards the tip. Press the tip to the baby's lips. If the sad face appears, your baby needs her medicine. If the happy face appears, your baby feels better. Slide the lever again to reset thermometer.

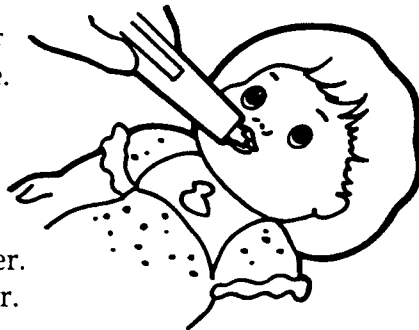

5

A little shot of "medicine" will fix her right up. This won't hurt a bit, baby!



6

Now give baby a bottle and a cuddle to keep her happy and healthy!



7

Store all in accessories case.

